


LABORATORY EQUIPMENT/ALL AFFECTED SURFACES EH&S CLEARANCE TESTING AND FM SERVICE FLOWCHART

Rev. 12/19
v.2

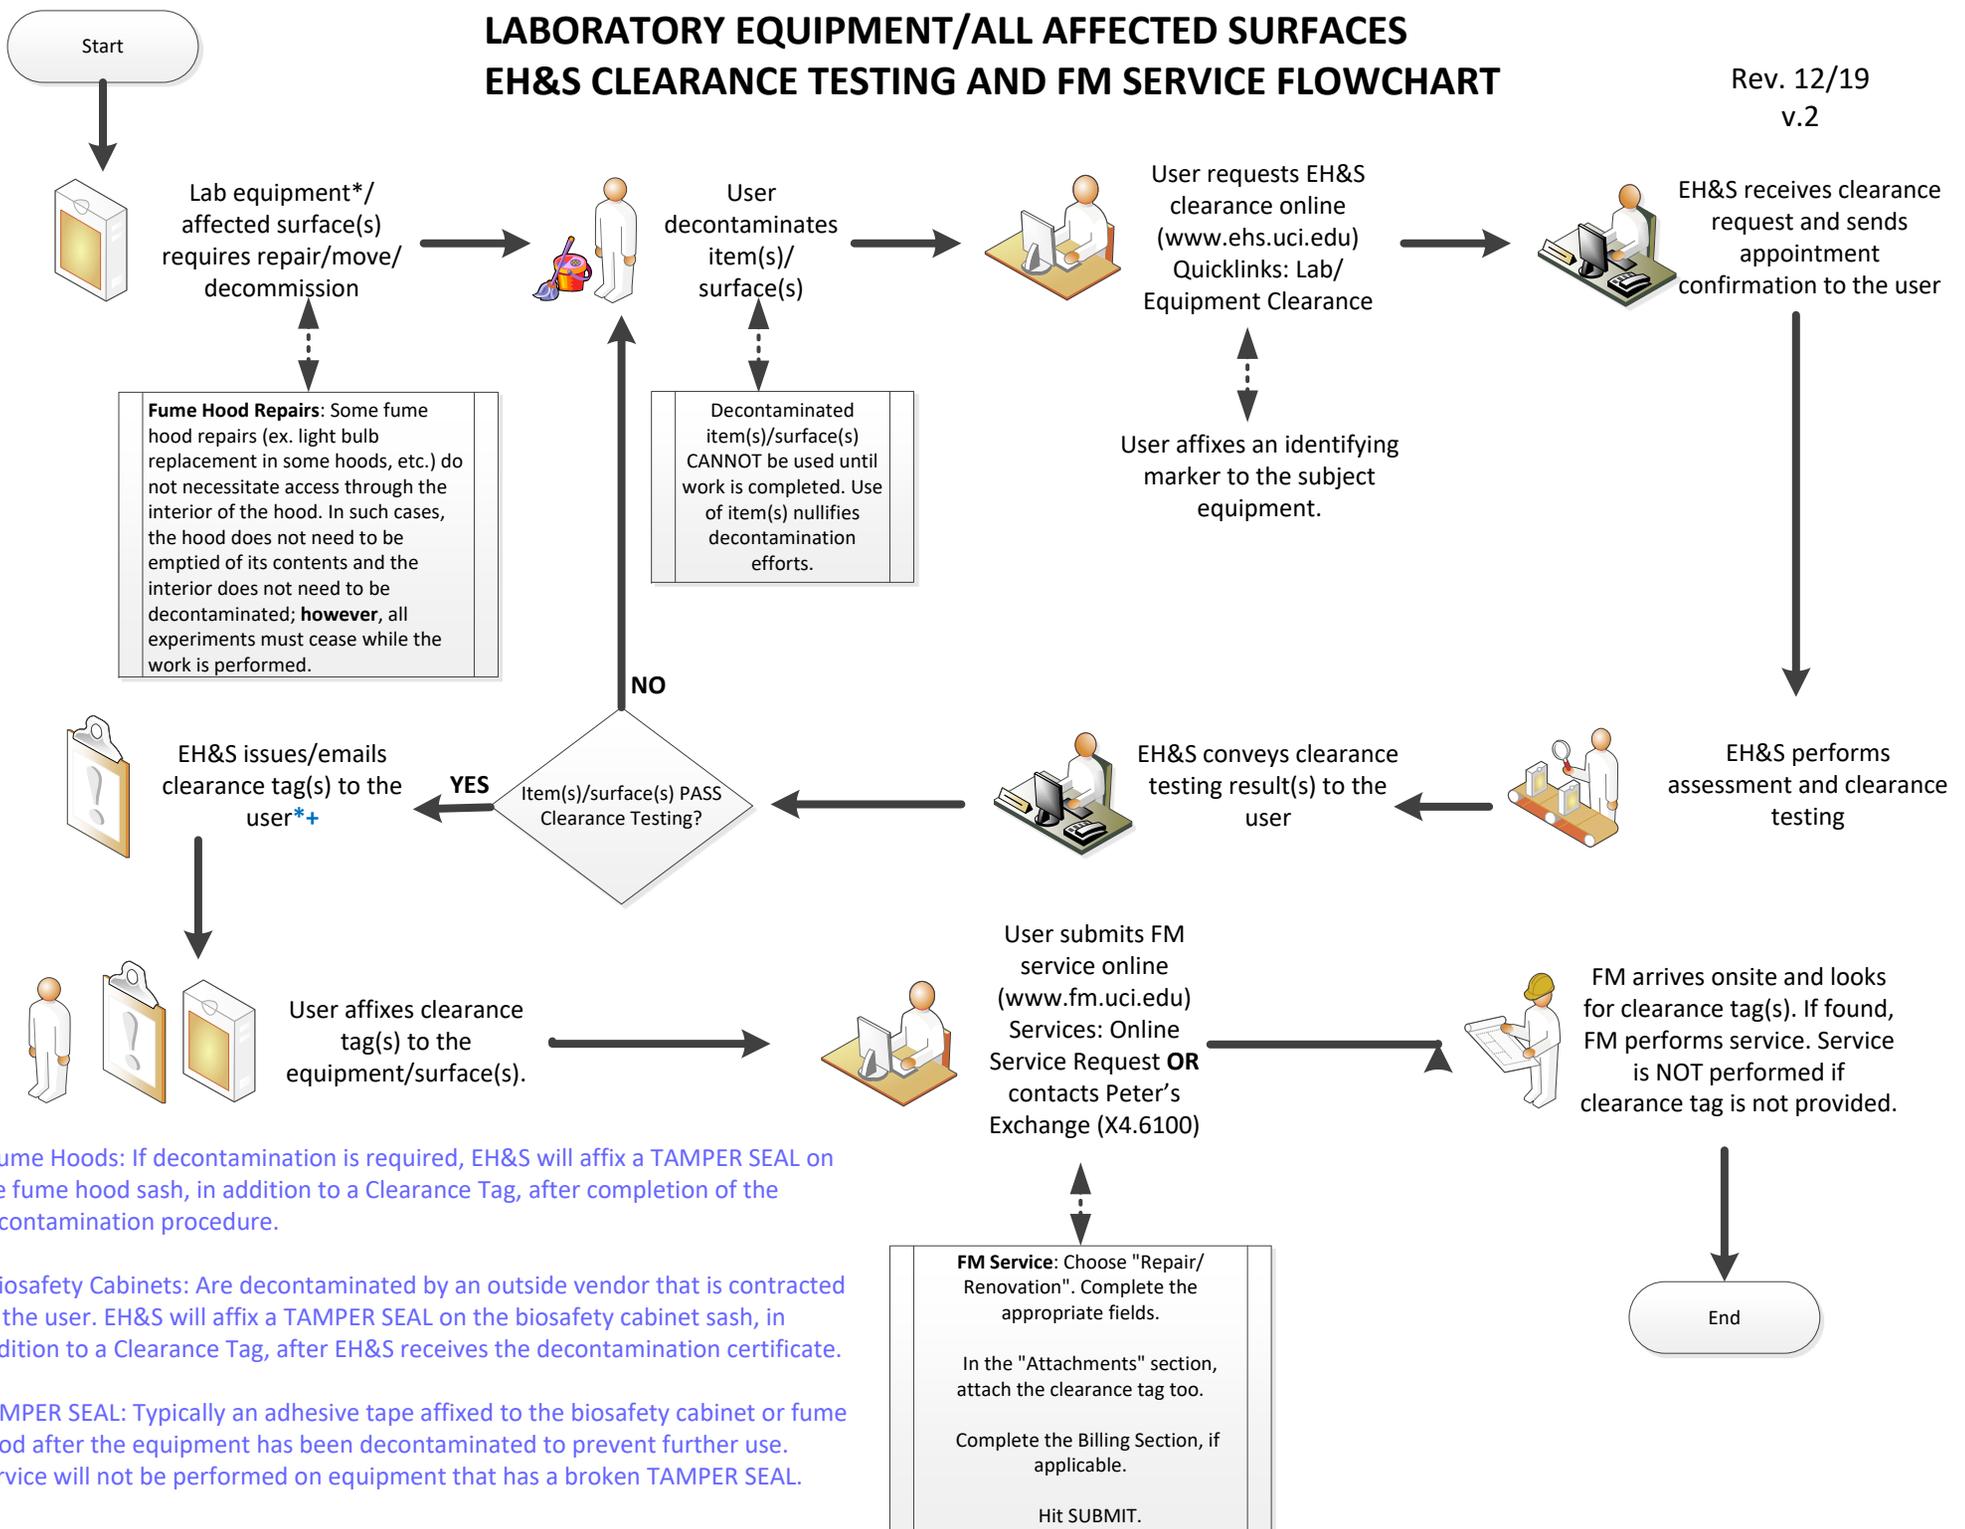

*Fume Hoods: If decontamination is required, EH&S will affix a TAMPER SEAL on the fume hood sash, in addition to a Clearance Tag, after completion of the decontamination procedure.

+Biosafety Cabinets: Are decontaminated by an outside vendor that is contracted by the user. EH&S will affix a TAMPER SEAL on the biosafety cabinet sash, in addition to a Clearance Tag, after EH&S receives the decontamination certificate.

TAMPER SEAL: Typically an adhesive tape affixed to the biosafety cabinet or fume hood after the equipment has been decontaminated to prevent further use. Service will not be performed on equipment that has a broken TAMPER SEAL.